

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306



Date: 06/24/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:37
INTERNAL STANDARD	VERIFIED	12:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:38
BLANK TEST	0.00	12:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:39
BLANK TEST	0.00	12:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:40
BLANK TEST	0.00	12:41

6/24/21
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 06/19/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:47
INTERNAL STANDARD	VERIFIED	08:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:48
BLANK TEST	0.00	08:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:49
BLANK TEST	0.00	08:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:50
BLANK TEST	0.00	08:51

② 471
6/19/21



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 06/13/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:50
INTERNAL STANDARD	VERIFIED	12:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:51
BLANK TEST	0.00	12:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:52
BLANK TEST	0.00	12:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:53
BLANK TEST	0.00	12:54

6/13/21
④ 471



RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 06/02/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:04
INTERNAL STANDARD	VERIFIED	13:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:05
BLANK TEST	0.00	13:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:06
BLANK TEST	0.00	13:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:07
BLANK TEST	0.00	13:08

① 471
 6/4/21



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 06/01/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:52
INTERNAL STANDARD	VERIFIED	10:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:53
BLANK TEST	0.00	10:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:54
BLANK TEST	0.00	10:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:55
BLANK TEST	0.00	10:56

6/1/21
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 05/25/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:21
INTERNAL STANDARD	VERIFIED	17:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:22
BLANK TEST	0.00	17:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:23
BLANK TEST	0.00	17:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:24
BLANK TEST	0.00	17:25

5/25/21
① 4H



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 05/18/2021

OPERATOR NAME:
ANTHONY E GIARDINA
Permit #: 35850
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020




Nominal = 0.10 g/210L

BLANK TEST	0.00	13:33
INTERNAL STANDARD	VERIFIED	13:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:33
BLANK TEST	0.00	13:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:34
BLANK TEST	0.00	13:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:36
BLANK TEST	0.00	13:36

05/18/21

Test

Lt. Anthony Giardina #430



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 05/10/2021




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:25
INTERNAL STANDARD	VERIFIED	16:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:25
BLANK TEST	0.00	16:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:26
BLANK TEST	0.00	16:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:27
BLANK TEST	0.00	16:28

5/10/21

② 477



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 05/10/2021




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:57
INTERNAL STANDARD	VERIFIED	15:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:57
BLANK TEST	0.00	15:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:58
BLANK TEST	0.00	15:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:59
BLANK TEST	0.00	16:00

5/10/21

①471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 05/03/2021




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:39
INTERNAL STANDARD	VERIFIED	10:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:40
BLANK TEST	0.00	10:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:41
BLANK TEST	0.00	10:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:42
BLANK TEST	0.00	10:43

5/3/21

471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 04/25/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:56
INTERNAL STANDARD	VERIFIED	18:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:57
BLANK TEST	0.00	18:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:58
BLANK TEST	0.00	18:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:59
BLANK TEST	0.00	19:00

4/25/21
① 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 04/20/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:31
INTERNAL STANDARD	VERIFIED	13:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:32
BLANK TEST	0.00	13:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:33
BLANK TEST	0.00	13:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:34
BLANK TEST	0.00	13:35

4/20/21
① 47



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 04/14/2021




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:30
INTERNAL STANDARD	VERIFIED	16:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:31
BLANK TEST	0.00	16:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:32
BLANK TEST	0.00	16:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:33
BLANK TEST	0.00	16:34

4/14/21

Q471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 04/10/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:55
INTERNAL STANDARD	VERIFIED	19:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:56
BLANK TEST	0.00	19:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:57
BLANK TEST	0.00	19:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:58
BLANK TEST	0.00	19:59

4/10/21
P471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 04/03/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:15
INTERNAL STANDARD	VERIFIED	19:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:16
BLANK TEST	0.00	19:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:17
BLANK TEST	0.00	19:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:18
BLANK TEST	0.00	19:19

4/3/21
② 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 03/26/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:53
INTERNAL STANDARD	VERIFIED	19:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:54
BLANK TEST	0.00	19:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:55
BLANK TEST	0.00	19:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:56
BLANK TEST	0.00	19:57

3/26/21
UH



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 03/20/2021




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:26
INTERNAL STANDARD	VERIFIED	14:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:27
BLANK TEST	0.00	14:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:28
BLANK TEST	0.00	14:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:29
BLANK TEST	0.00	14:30

3/20/21

47



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 03/13/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:23
INTERNAL STANDARD	VERIFIED	22:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:23
BLANK TEST	0.00	22:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:24
BLANK TEST	0.00	22:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:25
BLANK TEST	0.00	22:26

3/13/21
① 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 03/08/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:29
INTERNAL STANDARD	VERIFIED	10:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:30
BLANK TEST	0.00	10:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:31
BLANK TEST	0.00	10:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:32
BLANK TEST	0.00	10:33

① 47H
3/8/21



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 03/07/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:37
INTERNAL STANDARD	VERIFIED	14:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:37
BLANK TEST	0.00	14:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:38
BLANK TEST	0.00	14:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:40
BLANK TEST	0.00	14:40

3/7/21
[Signature]
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 03/02/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:58
INTERNAL STANDARD	VERIFIED	12:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:58
BLANK TEST	0.00	12:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:00
BLANK TEST	0.00	13:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:01
BLANK TEST	0.00	13:01

3/2/21
P 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 02/25/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:09
INTERNAL STANDARD	VERIFIED	15:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:09
BLANK TEST	0.00	15:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:11
BLANK TEST	0.00	15:12

2/25/21
[Signature]
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 02/19/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:32
INTERNAL STANDARD	VERIFIED	09:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:33
BLANK TEST	0.00	09:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:34
BLANK TEST	0.00	09:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:35
BLANK TEST	0.00	09:36

2/19/21
42014



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306


Date: 02/12/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:42
INTERNAL STANDARD	VERIFIED	21:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:43
BLANK TEST	0.00	21:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:44
BLANK TEST	0.00	21:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:45
BLANK TEST	0.00	21:46

2/12/21
① 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 02/10/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:15
INTERNAL STANDARD	VERIFIED	00:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:16
BLANK TEST	0.00	00:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:17
BLANK TEST	0.00	00:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:18
BLANK TEST	0.00	00:19

2/9/21
2047



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 02/02/2021




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:34
INTERNAL STANDARD	VERIFIED	11:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:35
BLANK TEST	0.00	11:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:36
BLANK TEST	0.00	11:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:37
BLANK TEST	0.00	11:38

① 471

2/2/2021



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 01/25/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:45
INTERNAL STANDARD	VERIFIED	16:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:45
BLANK TEST	0.00	16:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:46
BLANK TEST	0.00	16:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:48
BLANK TEST	0.00	16:48

① 471
1/25/2021




RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 01/18/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:58
INTERNAL STANDARD	VERIFIED	08:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:59
BLANK TEST	0.00	08:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:00
BLANK TEST	0.00	09:01
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:01
BLANK TEST	0.00	09:02

1/18/21

471



RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 01/10/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:24
INTERNAL STANDARD	VERIFIED	18:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:24
BLANK TEST	0.00	18:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:25
BLANK TEST	0.00	18:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:26
BLANK TEST	0.00	18:27

1/10/2021
① 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 01/04/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:37
INTERNAL STANDARD	VERIFIED	16:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:37
BLANK TEST	0.00	16:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:38
BLANK TEST	0.00	16:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:39
BLANK TEST	0.00	16:40

1/4/2021
②474

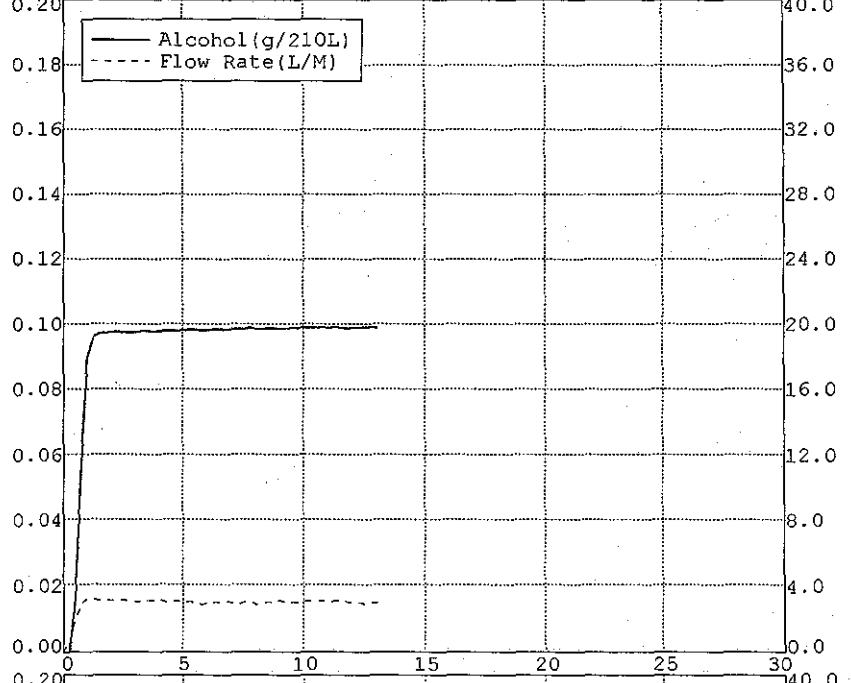

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/26/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:26
INTERNAL STANDARD	VERIFIED	00:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:28
BLANK TEST	0.00	00:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:29
BLANK TEST	0.00	00:30

12/26/20
①471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306



Date: 12/15/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:14
INTERNAL STANDARD	VERIFIED	21:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:14
BLANK TEST	0.00	21:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:15
BLANK TEST	0.00	21:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:16
BLANK TEST	0.00	21:17

12/15/20
① 47H



SOLUTION CHANGE

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/13/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:30
INTERNAL STANDARD	VERIFIED	01:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:30
BLANK TEST	0.00	01:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:32
BLANK TEST	0.00	01:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	01:33
BLANK TEST	0.00	01:33

① 471
12/13/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/11/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:07
INTERNAL STANDARD	VERIFIED	15:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:07
BLANK TEST	0.00	15:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:09
BLANK TEST	0.00	15:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:10
BLANK TEST	0.00	15:10

[Handwritten signature]
471
12/11/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/04/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:57
INTERNAL STANDARD	VERIFIED	11:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:58
BLANK TEST	0.00	11:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:59
BLANK TEST	0.00	12:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:00
BLANK TEST	0.00	12:01

Ⓟ 471
12/4/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 11/26/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:15
INTERNAL STANDARD	VERIFIED	21:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:16
BLANK TEST	0.00	21:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	21:17
BLANK TEST	0.00	21:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:18
BLANK TEST	0.00	21:19

11/26/20
471



RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 11/19/2020

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:53
INTERNAL STANDARD	VERIFIED	12:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:54
BLANK TEST	0.00	12:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:55
BLANK TEST	0.00	12:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:56
BLANK TEST	0.00	12:57

11/19/20
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 11/15/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:11
INTERNAL STANDARD	VERIFIED	03:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:11
BLANK TEST	0.00	03:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:12
BLANK TEST	0.00	03:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:13
BLANK TEST	0.00	03:14

11/15/20
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 11/11/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:49
INTERNAL STANDARD	VERIFIED	23:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:50
BLANK TEST	0.00	23:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:51
BLANK TEST	0.00	23:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:52
BLANK TEST	0.00	23:53

11/11/20
B 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 11/05/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:25
INTERNAL STANDARD	VERIFIED	09:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:26
BLANK TEST	0.00	09:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:27
BLANK TEST	0.00	09:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:28
BLANK TEST	0.00	09:29

11/5/20
D471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/31/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:14
INTERNAL STANDARD	VERIFIED	23:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:14
BLANK TEST	0.00	23:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:15
BLANK TEST	0.00	23:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:17
BLANK TEST	0.00	23:17

0471
10/31/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/30/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:05
INTERNAL STANDARD	VERIFIED	19:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:05
BLANK TEST	0.00	19:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:06
BLANK TEST	0.00	19:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:07
BLANK TEST	0.00	19:08

① 471
10/30/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/27/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:38
INTERNAL STANDARD	VERIFIED	20:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:38
BLANK TEST	0.00	20:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:39
BLANK TEST	0.00	20:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:41
BLANK TEST	0.00	20:41

10/27/20
① 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 10/27/2020


OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:34
INTERNAL STANDARD	VERIFIED	20:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD INTERFERENCE		20:34

Blank Error

10/27/20
DU71
Blank error



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 10/20/2020





OPERATOR NAME:
MICHAEL T ANTON
Permit #: 36793
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:28
INTERNAL STANDARD	VERIFIED	18:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	18:28
BLANK TEST	0.00	18:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:29
BLANK TEST	0.00	18:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:30
BLANK TEST	0.00	18:31

MA450

10/20/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 10/12/2020




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:39
INTERNAL STANDARD	VERIFIED	16:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:39
BLANK TEST	0.00	16:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:40
BLANK TEST	0.00	16:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:42
BLANK TEST	0.00	16:42

①471

10/12/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/09/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:24
INTERNAL STANDARD	VERIFIED	08:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:24
BLANK TEST	0.00	08:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:25
BLANK TEST	0.00	08:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:26
BLANK TEST	0.00	08:27

10/9/20
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/05/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:23
INTERNAL STANDARD	VERIFIED	14:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:23
BLANK TEST	0.00	14:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:25
BLANK TEST	0.00	14:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:26
BLANK TEST	0.00	14:27

④ 471
10/5/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/30/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:42
INTERNAL STANDARD	VERIFIED	10:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:43
BLANK TEST	0.00	10:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:44
BLANK TEST	0.00	10:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:45
BLANK TEST	0.00	10:46

0471
9/30/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/23/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:27
INTERNAL STANDARD	VERIFIED	10:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:27
BLANK TEST	0.00	10:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:28
BLANK TEST	0.00	10:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:30
BLANK TEST	0.00	10:30

471
9/23/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/17/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:38
INTERNAL STANDARD	VERIFIED	19:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:38
BLANK TEST	0.00	19:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:39
BLANK TEST	0.00	19:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	19:40
BLANK TEST	0.00	19:41

471
9/17/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/08/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:24
INTERNAL STANDARD	VERIFIED	12:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:25
BLANK TEST	0.00	12:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:26
BLANK TEST	0.00	12:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:27
BLANK TEST	0.00	12:28

① 471
9/8/2020



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/29/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:43
INTERNAL STANDARD	VERIFIED	23:43
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:44
BLANK TEST	0.00	23:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:45
BLANK TEST	0.00	23:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:46
BLANK TEST	0.00	23:47

471
8/29/20

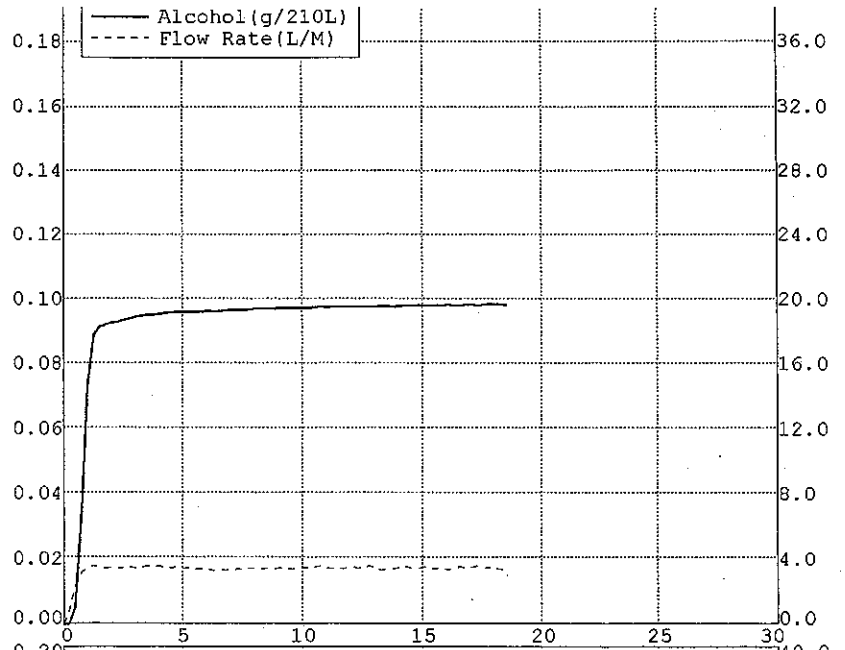

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/25/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:46
INTERNAL STANDARD	VERIFIED	10:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:46
BLANK TEST	0.00	10:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:47
BLANK TEST	0.00	10:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:49
BLANK TEST	0.00	10:49

8/25/2020
① 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/22/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:11
INTERNAL STANDARD	VERIFIED	23:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:11
BLANK TEST	0.00	23:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:12
BLANK TEST	0.00	23:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	23:14
BLANK TEST	0.00	23:14

8/22/20
①47



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/14/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:11
INTERNAL STANDARD	VERIFIED	16:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:11
BLANK TEST	0.00	16:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:12
BLANK TEST	0.00	16:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:14
BLANK TEST	0.00	16:14

8/14/20
P
471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/10/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:55
INTERNAL STANDARD	VERIFIED	19:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:56
BLANK TEST	0.00	19:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:57
BLANK TEST	0.00	19:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:58
BLANK TEST	0.00	19:59

8/10/20
① 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/02/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:22
INTERNAL STANDARD	VERIFIED	18:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:23
BLANK TEST	0.00	18:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:24
BLANK TEST	0.00	18:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:25
BLANK TEST	0.00	18:26

8/2/2020
A.F.S.



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/28/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:53
INTERNAL STANDARD	VERIFIED	10:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:53
BLANK TEST	0.00	10:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:54
BLANK TEST	0.00	10:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:56
BLANK TEST	0.00	10:56

① 471
7/28/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/23/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:33
INTERNAL STANDARD	VERIFIED	20:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:34
BLANK TEST	0.00	20:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:35
BLANK TEST	0.00	20:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	20:36
BLANK TEST	0.00	20:37

471
7/23/20



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/23/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:36
INTERNAL STANDARD	VERIFIED	19:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:36
BLANK TEST	0.00	19:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:37
BLANK TEST	0.00	19:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:39
BLANK TEST	0.00	19:39

PH
7/23/20

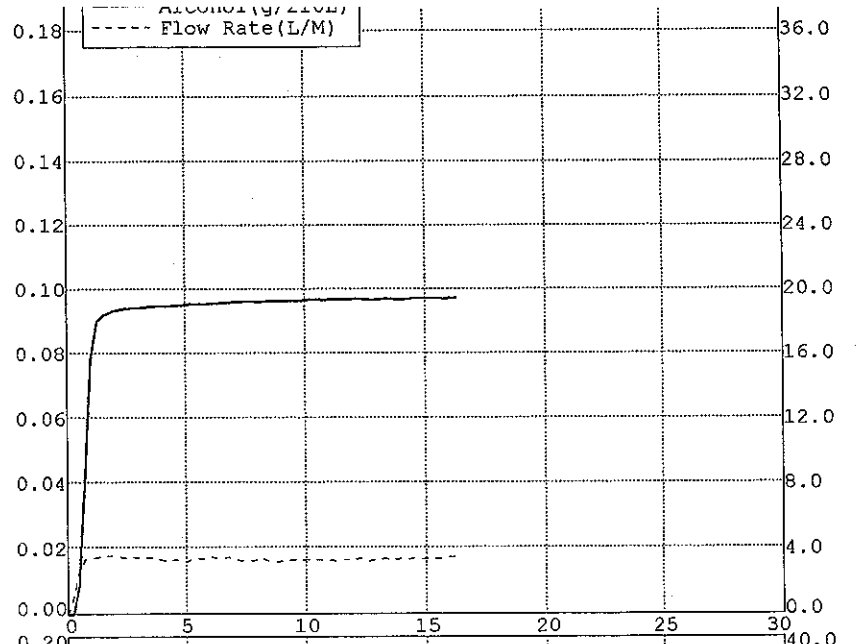

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 07/15/2020




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:31
INTERNAL STANDARD	VERIFIED	19:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:32
BLANK TEST	0.00	19:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:33
BLANK TEST	0.00	19:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:34
BLANK TEST	0.00	19:35

0471

7/15/20






RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 07/09/2020

OPERATOR NAME:
ANTHONY E GIARDINA
Permit #: 35850
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:52
INTERNAL STANDARD	VERIFIED	13:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:53
BLANK TEST	0.00	13:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:54
BLANK TEST	0.00	13:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:55
BLANK TEST	0.00	13:56



Test 7/9/20
St. AS430

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/02/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:30
INTERNAL STANDARD	VERIFIED	21:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:30
BLANK TEST	0.00	21:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:32
BLANK TEST	0.00	21:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:33
BLANK TEST	0.00	21:34

7/2/20
0471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 06/29/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:34
INTERNAL STANDARD	VERIFIED	22:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:35
BLANK TEST	0.00	22:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:36
BLANK TEST	0.00	22:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:37
BLANK TEST	0.00	22:38

P 471



RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 06/25/2020

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:08
INTERNAL STANDARD	VERIFIED	16:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:09
BLANK TEST	0.00	16:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:10
BLANK TEST	0.00	16:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:11
BLANK TEST	0.00	16:12

①471

6/25/2020

