

SUPERVISOR TEST




RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306

Date: 12/31/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21390

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 11:37 |
| INTERNAL STANDARD | VERIFIED | 11:37 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 11:38 |
| BLANK TEST | 0.00 | 11:38 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 11:39 |
| BLANK TEST | 0.00 | 11:39 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 11:40 |
| BLANK TEST | 0.00 | 11:41 |

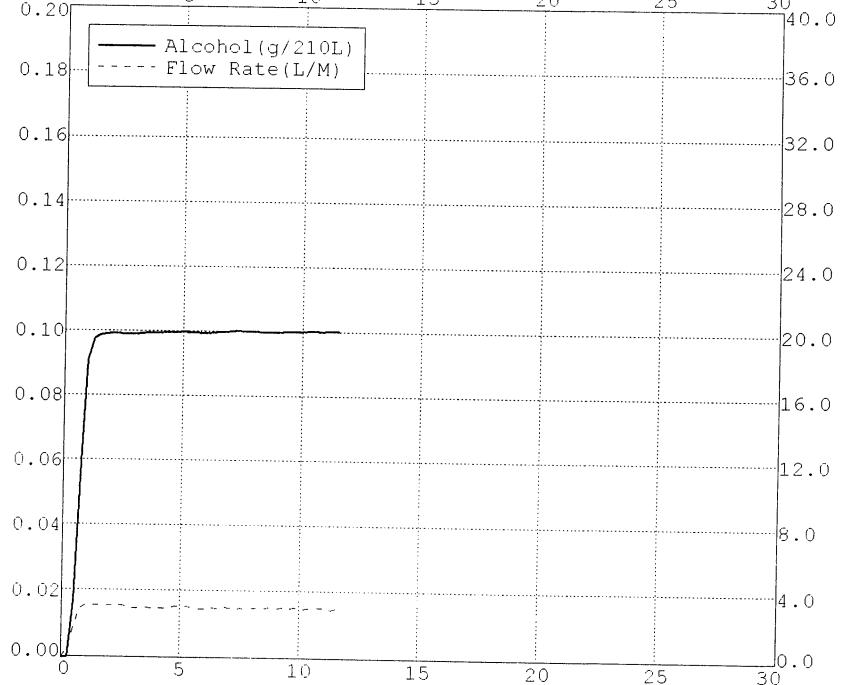

SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 12/29/2021




OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 08:37 |
| INTERNAL STANDARD | VERIFIED | 08:37 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 08:37 |
| BLANK TEST | 0.00 | 08:38 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:38 |
| BLANK TEST | 0.00 | 08:39 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 08:39 |
| BLANK TEST | 0.00 | 08:40 |

12/29/21

471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/23/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 22:19 |
| INTERNAL STANDARD | VERIFIED | 22:19 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 22:19 |
| BLANK TEST | 0.00 | 22:20 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 22:20 |
| BLANK TEST | 0.00 | 22:21 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 22:21 |
| BLANK TEST | 0.00 | 22:22 |

12/23/21
①47H

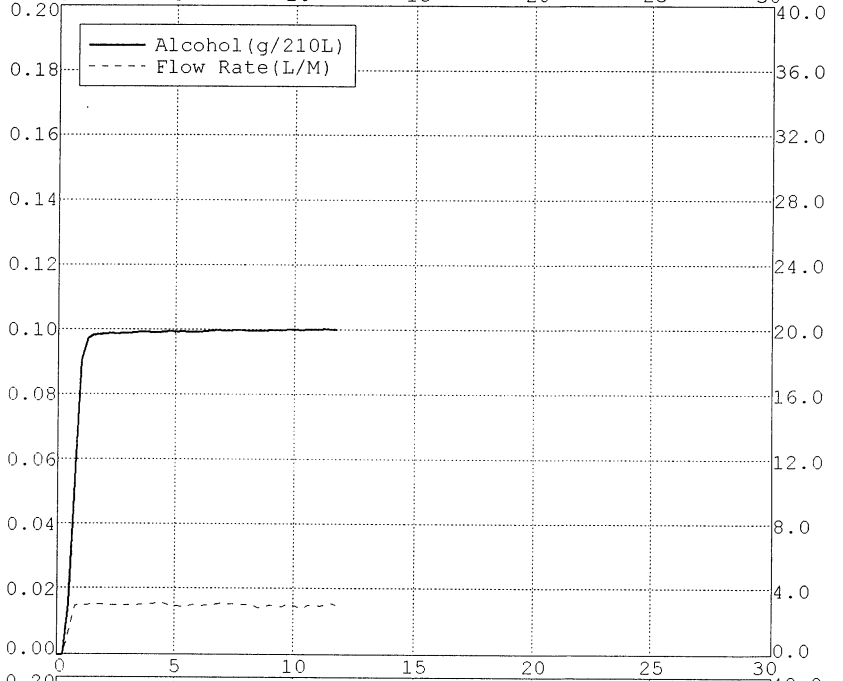

SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/21/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 21:11 |
| INTERNAL STANDARD | VERIFIED | 21:11 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:12 |
| BLANK TEST | 0.00 | 21:13 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:13 |
| BLANK TEST | 0.00 | 21:14 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 21:14 |
| BLANK TEST | 0.00 | 21:15 |

12/21/21
② 471



SUPERVISOR TEST

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306

Date: 12/16/2021




OPERATOR NAME:
 ANTHONY E GIARDINA
 Permit #: 35850
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21390

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 11:00 |
| INTERNAL STANDARD | VERIFIED | 11:00 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 11:01 |
| BLANK TEST | 0.00 | 11:02 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 11:02 |
| BLANK TEST | 0.00 | 11:03 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 11:03 |
| BLANK TEST | 0.00 | 11:04 |

WEEKLY TEST

Lt AG 430



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/08/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21390

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 20:05 |
| INTERNAL STANDARD | VERIFIED | 20:05 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 20:05 |
| BLANK TEST | 0.00 | 20:06 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 20:06 |
| BLANK TEST | 0.00 | 20:07 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 20:08 |
| BLANK TEST | 0.00 | 20:08 |

D 471



SOLUTION CHANGE

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 12/06/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21390

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 17:07 |
| INTERNAL STANDARD | VERIFIED | 17:07 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:07 |
| BLANK TEST | 0.00 | 17:08 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:08 |
| BLANK TEST | 0.00 | 17:09 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 17:09 |
| BLANK TEST | 0.00 | 17:10 |

(Signature)
 12/6/21



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 12/01/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 08:42 |
| INTERNAL STANDARD | VERIFIED | 08:42 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:42 |
| BLANK TEST | 0.00 | 08:43 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:43 |
| BLANK TEST | 0.00 | 08:44 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 08:44 |
| BLANK TEST | 0.00 | 08:45 |

12/1/21
② 471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306



Date: 11/24/2021

OPERATOR NAME:
JAMES TESSEYMAN
Permit #: 47783
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 11:55 |
| INTERNAL STANDARD | VERIFIED | 11:55 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 11:55 |
| BLANK TEST | 0.00 | 11:56 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 11:56 |
| BLANK TEST | 0.00 | 11:57 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 11:58 |
| BLANK TEST | 0.00 | 11:58 |

JT
11/24/2021



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 11/17/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 16:00 |
| INTERNAL STANDARD | VERIFIED | 16:00 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 16:00 |
| BLANK TEST | 0.00 | 16:01 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 16:02 |
| BLANK TEST | 0.00 | 16:02 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 16:03 |
| BLANK TEST | 0.00 | 16:04 |

11/17/21
[Signature] 471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 11/14/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 15:14 |
| INTERNAL STANDARD | VERIFIED | 15:14 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 15:15 |
| BLANK TEST | 0.00 | 15:16 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 15:16 |
| BLANK TEST | 0.00 | 15:17 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 15:17 |
| BLANK TEST | 0.00 | 15:18 |

11/14/21
②471



SOLUTION CHANGE

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 11/10/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 17:30 |
| INTERNAL STANDARD | VERIFIED | 17:30 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:30 |
| BLANK TEST | 0.00 | 17:31 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:31 |
| BLANK TEST | 0.00 | 17:32 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:33 |
| BLANK TEST | 0.00 | 17:33 |

Ⓟ 471
11/10/21



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/30/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 10:09 |
| INTERNAL STANDARD | VERIFIED | 10:09 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 10:09 |
| BLANK TEST | 0.00 | 10:10 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 10:10 |
| BLANK TEST | 0.00 | 10:11 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 10:11 |
| BLANK TEST | 0.00 | 10:12 |

10/30/21
②471



SUPERVISOR TEST

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306


Date: 10/25/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 16:21 |
| INTERNAL STANDARD | VERIFIED | 16:21 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 16:21 |
| BLANK TEST | 0.00 | 16:22 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 16:23 |
| BLANK TEST | 0.00 | 16:23 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 16:24 |
| BLANK TEST | 0.00 | 16:24 |

10/25/21
P47



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/21/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 14:26 |
| INTERNAL STANDARD | VERIFIED | 14:26 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 14:26 |
| BLANK TEST | 0.00 | 14:27 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 14:27 |
| BLANK TEST | 0.00 | 14:28 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 14:29 |
| BLANK TEST | 0.00 | 14:29 |

10/21/21
DUZ



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/17/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 13:24 |
| INTERNAL STANDARD | VERIFIED | 13:25 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 13:25 |
| BLANK TEST | 0.00 | 13:26 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 13:26 |
| BLANK TEST | 0.00 | 13:27 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 13:27 |
| BLANK TEST | 0.00 | 13:28 |

10/17/21
0471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/14/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 08:46 |
| INTERNAL STANDARD | VERIFIED | 08:46 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:46 |
| BLANK TEST | 0.00 | 08:47 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:47 |
| BLANK TEST | 0.00 | 08:48 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 08:49 |
| BLANK TEST | 0.00 | 08:49 |

10/14/21
Q47



SUPERVISOR TEST

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306

Date: 10/08/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21280




Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 17:06 |
| INTERNAL STANDARD | VERIFIED | 17:06 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:06 |
| BLANK TEST | 0.00 | 17:07 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:07 |
| BLANK TEST | 0.00 | 17:08 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:08 |
| BLANK TEST | 0.00 | 17:09 |

10/8/21

Ⓟ

471



SOLUTION CHANGE

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 10/05/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21280

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 10:11 |
| INTERNAL STANDARD | VERIFIED | 10:11 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:12 |
| BLANK TEST | 0.00 | 10:13 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 10:13 |
| BLANK TEST | 0.00 | 10:14 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 10:14 |
| BLANK TEST | 0.00 | 10:15 |

10/5/21
0471



SUPERVISOR TEST




RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 10/01/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 12:20 |
| INTERNAL STANDARD | VERIFIED | 12:20 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 12:21 |
| BLANK TEST | 0.00 | 12:21 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 12:22 |
| BLANK TEST | 0.00 | 12:23 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 12:23 |
| BLANK TEST | 0.00 | 12:24 |



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/26/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 16:26 |
| INTERNAL STANDARD | VERIFIED | 16:26 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 16:26 |
| BLANK TEST | 0.00 | 16:27 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 16:28 |
| BLANK TEST | 0.00 | 16:28 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 16:29 |
| BLANK TEST | 0.00 | 16:30 |

9/26/21
①471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/23/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 01:13 |
| INTERNAL STANDARD | VERIFIED | 01:14 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 01:14 |
| BLANK TEST | 0.00 | 01:15 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 01:15 |
| BLANK TEST | 0.00 | 01:16 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 01:16 |
| BLANK TEST | 0.00 | 01:17 |

471
9/23/21



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/18/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 15:45 |
| INTERNAL STANDARD | VERIFIED | 15:45 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 15:46 |
| BLANK TEST | 0.00 | 15:46 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 15:47 |
| BLANK TEST | 0.00 | 15:48 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 15:48 |
| BLANK TEST | 0.00 | 15:49 |

9/18/21
②47/



SOLUTION CHANGE

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/15/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 17:41 |
| INTERNAL STANDARD | VERIFIED | 17:41 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.09 | 17:42 |
| BLANK TEST | 0.00 | 17:43 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 17:43 |
| BLANK TEST | 0.00 | 17:44 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 17:45 |
| BLANK TEST | 0.00 | 17:45 |

*9/15/21
② 477*

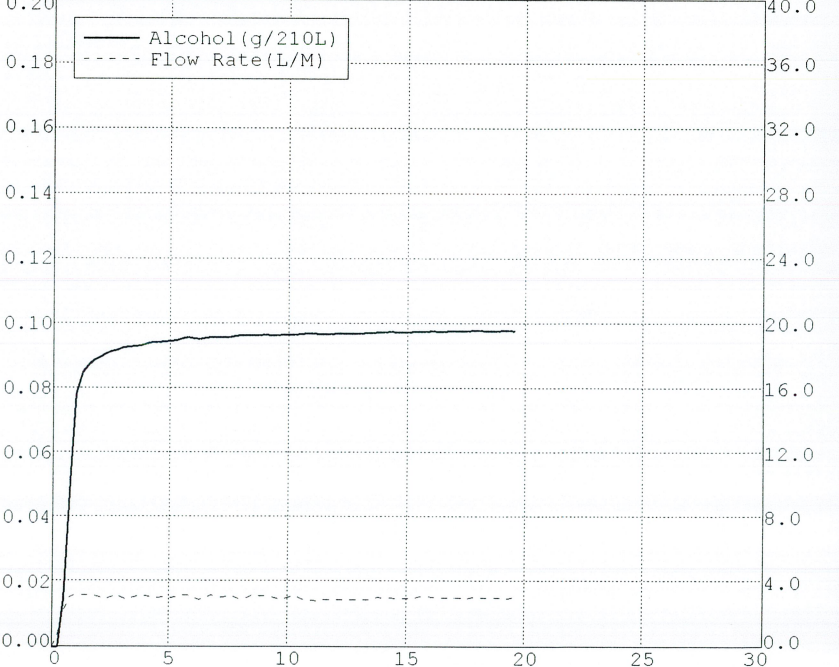

SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 09/13/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 14:22 |
| INTERNAL STANDARD | VERIFIED | 14:22 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 14:22 |
| BLANK TEST | 0.00 | 14:23 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.09 | 14:23 |
| BLANK TEST | 0.00 | 14:24 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 14:25 |
| BLANK TEST | 0.00 | 14:25 |

9/13/21
P 471

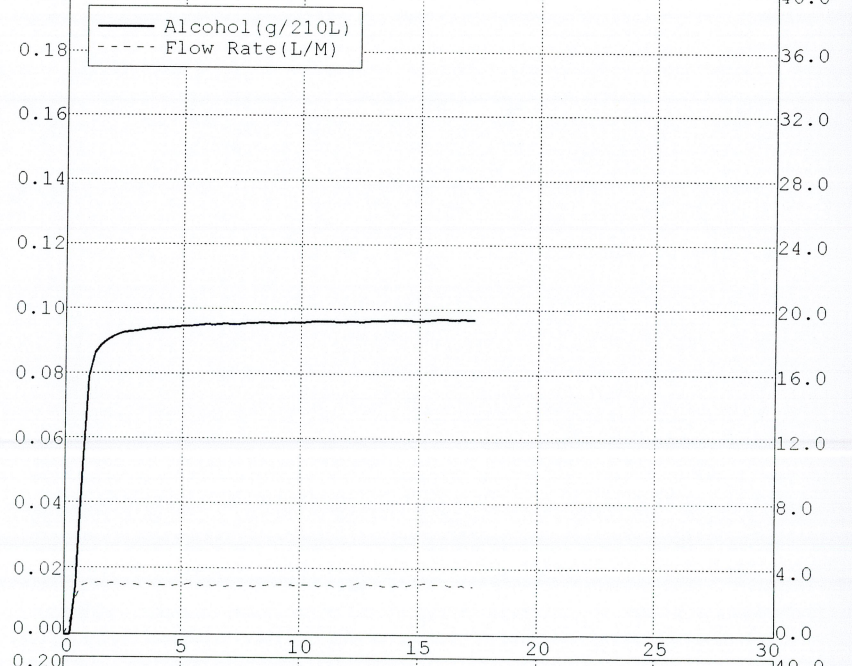

SOLUTION CHANGE

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 09/07/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 19:23 |
| INTERNAL STANDARD | VERIFIED | 19:23 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 19:23 |
| BLANK TEST | 0.00 | 19:24 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 19:25 |
| BLANK TEST | 0.00 | 19:25 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 19:26 |
| BLANK TEST | 0.00 | 19:27 |

9/7/21
 471



SUPERVISOR TEST

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 09/07/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 16:24 |
| INTERNAL STANDARD | VERIFIED | 16:24 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 16:25 |
| BLANK TEST | 0.00 | 16:26 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 16:26 |
| BLANK TEST | 0.00 | 16:27 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 16:27 |
| BLANK TEST | 0.00 | 16:28 |

9/7/21
 047



SUPERVISOR TEST

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 08/31/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:49 |
| INTERNAL STANDARD | VERIFIED | 18:49 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 18:49 |
| BLANK TEST | 0.00 | 18:50 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 18:50 |
| BLANK TEST | 0.00 | 18:51 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 18:52 |
| BLANK TEST | 0.00 | 18:52 |

8/31/21
 474



SUPERVISOR TEST

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 08/24/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 18:52 |
| INTERNAL STANDARD | VERIFIED | 18:52 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 18:53 |
| BLANK TEST | 0.00 | 18:54 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 18:54 |
| BLANK TEST | 0.00 | 18:55 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 18:55 |
| BLANK TEST | 0.00 | 18:56 |

8/24/21
 477



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/19/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 13:12 |
| INTERNAL STANDARD | VERIFIED | 13:12 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 13:13 |
| BLANK TEST | 0.00 | 13:14 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 13:14 |
| BLANK TEST | 0.00 | 13:15 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 13:15 |
| BLANK TEST | 0.00 | 13:16 |

8/19/21
① 471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/16/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 10:07 |
| INTERNAL STANDARD | VERIFIED | 10:07 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:08 |
| BLANK TEST | 0.00 | 10:09 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:09 |
| BLANK TEST | 0.00 | 10:10 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:10 |
| BLANK TEST | 0.00 | 10:11 |

8/16/21
① 471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/10/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 11:57 |
| INTERNAL STANDARD | VERIFIED | 11:57 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 11:58 |
| BLANK TEST | 0.00 | 11:59 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 11:59 |
| BLANK TEST | 0.00 | 12:00 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 12:00 |
| BLANK TEST | 0.00 | 12:01 |

D471
8/10/21



SOLUTION CHANGE

RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306




Date: 08/05/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 13:58 |
| INTERNAL STANDARD | VERIFIED | 13:59 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 13:59 |
| BLANK TEST | 0.00 | 14:00 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 14:00 |
| BLANK TEST | 0.00 | 14:01 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 14:01 |
| BLANK TEST | 0.00 | 14:02 |

8/5/21
 P47



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 08/01/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 10:49 |
| INTERNAL STANDARD | VERIFIED | 10:49 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:50 |
| BLANK TEST | 0.00 | 10:50 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:51 |
| BLANK TEST | 0.00 | 10:52 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:52 |
| BLANK TEST | 0.00 | 10:53 |

8/1/21
D471



SUPERVISOR TEST




RAMAPO TOWN
 POLICE DEPT
 DATAMASTER dmt: 116306

Date: 07/25/2021

OPERATOR NAME:
 ANDRES F SANCHEZ
 Permit #: 42014
 Operator Agency/Dept: RAMAPO TOWN PD
 Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 20:12 |
| INTERNAL STANDARD | VERIFIED | 20:12 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 20:12 |
| BLANK TEST | 0.00 | 20:13 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 20:13 |
| BLANK TEST | 0.00 | 20:14 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 20:14 |
| BLANK TEST | 0.00 | 20:15 |

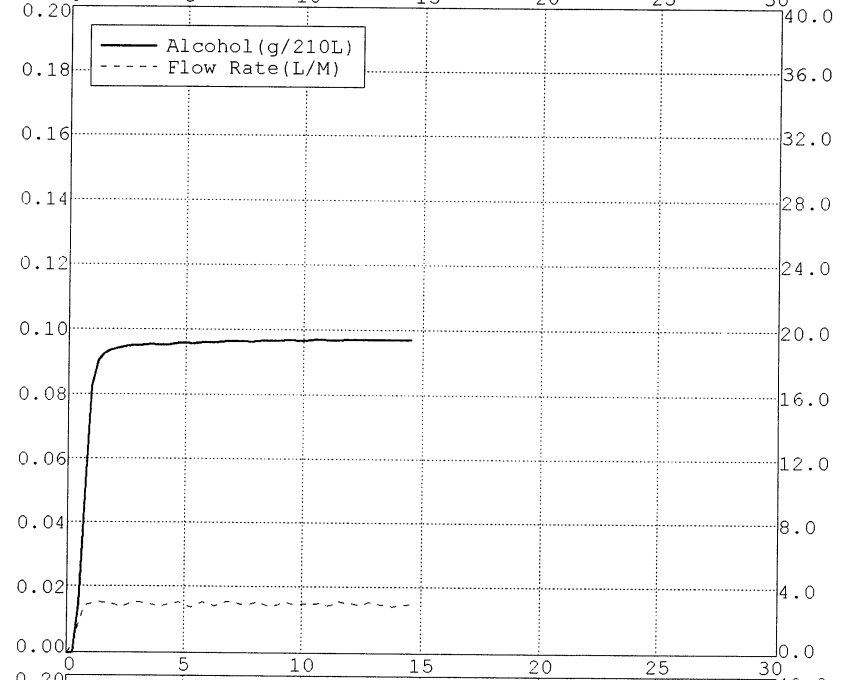

SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/22/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 11:23 |
| INTERNAL STANDARD | VERIFIED | 11:23 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 11:23 |
| BLANK TEST | 0.00 | 11:24 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 11:25 |
| BLANK TEST | 0.00 | 11:25 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 11:26 |
| BLANK TEST | 0.00 | 11:26 |

7/22/21
431



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/19/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 08:21 |
| INTERNAL STANDARD | VERIFIED | 08:21 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 08:21 |
| BLANK TEST | 0.00 | 08:22 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 08:22 |
| BLANK TEST | 0.00 | 08:23 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 08:23 |
| BLANK TEST | 0.00 | 08:24 |

7/19/21
471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/14/2021

OPERATOR NAME:
JAMES E TESSEYMAN
Permit #: 47783
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 10:00 |
| INTERNAL STANDARD | VERIFIED | 10:00 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 10:01 |
| BLANK TEST | 0.00 | 10:01 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:02 |
| BLANK TEST | 0.00 | 10:02 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 10:03 |
| BLANK TEST | 0.00 | 10:04 |

7/14/21
JT 492



SOLUTION CHANGE

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306




Date: 07/04/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 16:41 |
| INTERNAL STANDARD | VERIFIED | 16:41 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 16:42 |
| BLANK TEST | 0.00 | 16:42 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 16:43 |
| BLANK TEST | 0.00 | 16:44 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 16:44 |
| BLANK TEST | 0.00 | 16:45 |

7/4/21
0471



SUPERVISOR TEST

RAMAPO TOWN
POLICE DEPT
DATAMASTER dmt: 116306

Date: 07/02/2021

OPERATOR NAME:
ANDRES F SANCHEZ
Permit #: 42014
Operator Agency/Dept: RAMAPO TOWN PD
Reference Standard #: 21100

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 12:39 |
| INTERNAL STANDARD | VERIFIED | 12:39 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 12:39 |
| BLANK TEST | 0.00 | 12:40 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 12:40 |
| BLANK TEST | 0.00 | 12:41 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.09 | 12:42 |
| BLANK TEST | 0.00 | 12:42 |

7/2/21
(P) 471

